# Installation Instructions

## 9A31500* Welch Allyn Light Bracket

***(Use w/ 48700 Light)***

### Intended Use

To mount a Welch Allyn 48700 Light to 222 exam table *(on patient's left side)*.

### Kit Components

| *Description* | *Part Number* | *Qty* |
|---|---|---|
| Bracket | 030-1429-50 | 1 |
| Bottom Plate | 050-5579-50 | 1 |
| Screws: | | |
| *#10-24 x 1/2"* | 040-0010-129 | 4 |
| *#10-32 x 3/8"* | 040-0010-74 | 2 |
| Nuts: | | |
| *#10-32, Esna thin* | 041-0010-12 | 2 |

### Installation

(1) Insert bottom plate (1, Figure 1) thru slot in bracket (2) and secure with two 1/2" screws (3).

(2) Lift seat section; pull footrest and stirrups out.

(3) Remove screw (4) and insert front of bracket (2) between upperwrap & drawer housing.

(4) Align hole in bracket (2) with holes in upperwrap and drawer housing; then install screw (4).

(5) Remove screw (5) and move back of bracket (2) between upperwrap & drawer housing.

(6) Align hole in bracket (2) with holes in upperwrap and drawer housing; then install screw (5).

(7) Remove drawer.

(8) Secure bracket (2) to bottom of drawer housing with two 3/8" screws (6) and two nuts (7).

**NOTE**

There are two screws *(#10-24 x 1/2")* provided to mount the Welch Allyn 48700 light to the bracket.

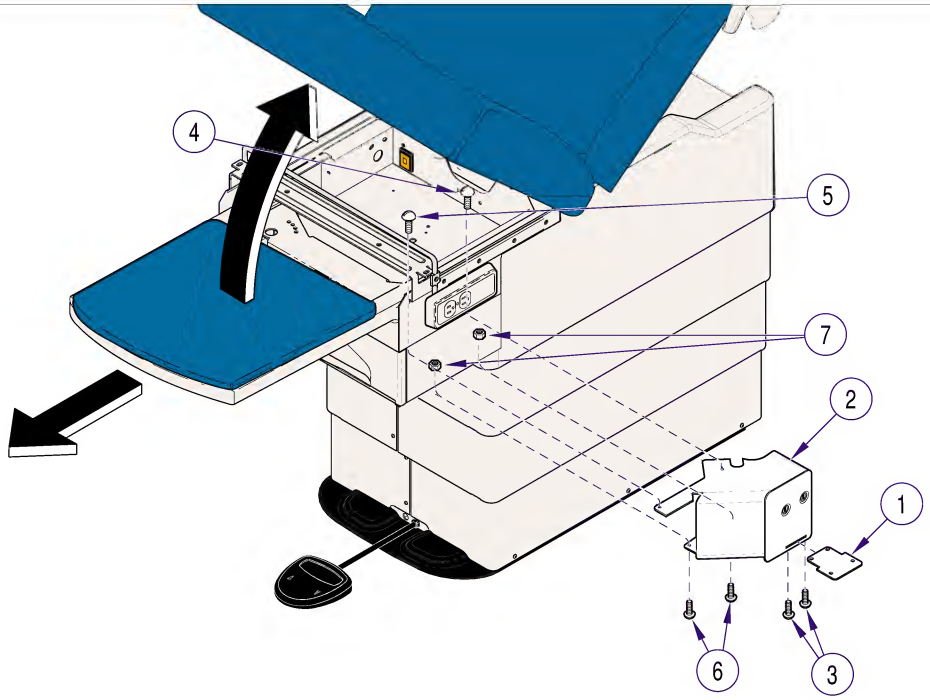


**Figure 1. Welch-Allyn Bracket Installation**

MA606500i

© Midmark Corporation 2002